



Instruction for Use

Blood Collection with S-Monovette® for use with Roche Multiplate® Analyser


Blood Collection with S-Monovette® Hirudin and S-Monovette® Needle

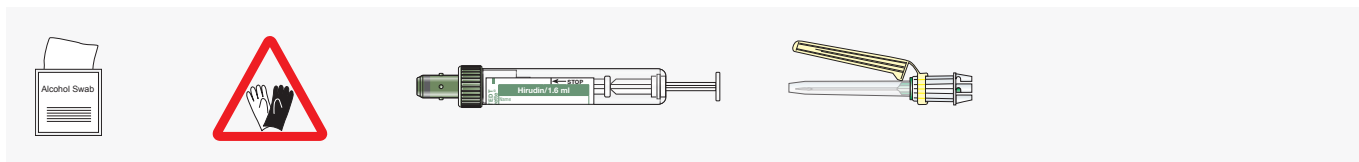


Aspiration method – The gentle method for increased patient comfort

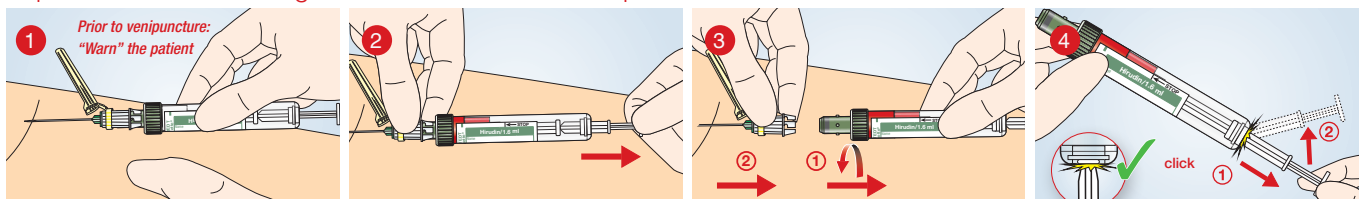


Vacuum method – Always a fresh vacuum

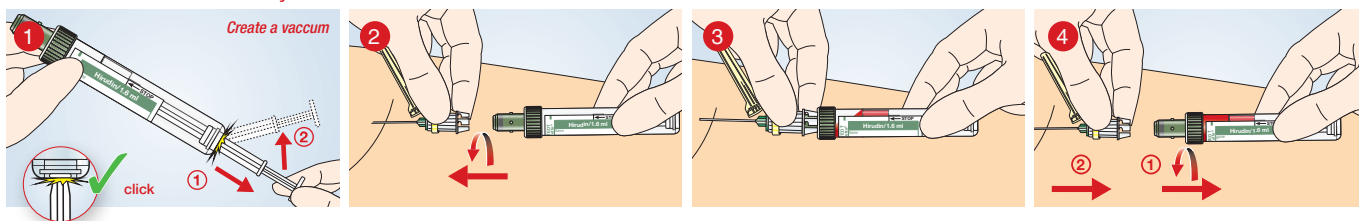

Blood Collection with S-Monovette® Hirudin and Vacuum Needle & Vacuum Holder

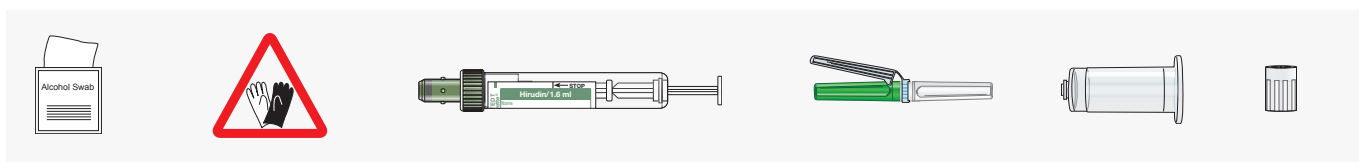

Vacuum method – Always a fresh vacuum

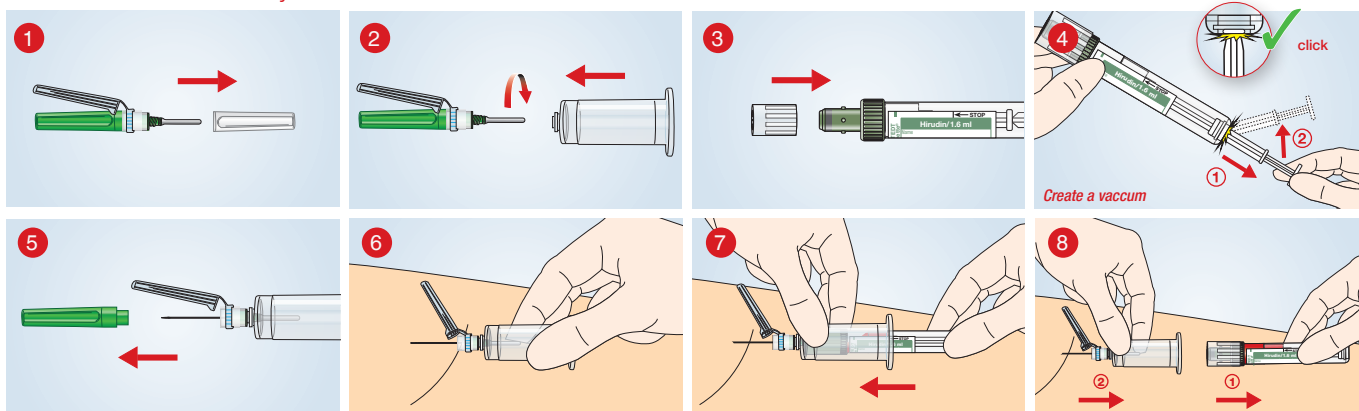

SARSTEDT AG & Co. KG
 P.O. Box 12 20
 D-51582 Nümbrecht
 Phone +49 2293 305 - 0
 Fax +49 2293 305 - 3992
 export@sarstedt.com
 www.sarstedt.com

